

Kennzeichnung Prüfstelle


Test Facility RMA RMA

Meter Data

22.11.2022

Manufacturer:	RMG	Flange Type:	ANSI 800
Serial Number:	828193	Pressure (bar a):	46
Year:	2022	Pulse Value (Imp/m³):	1714.000
Meter Size:	Type 1 TME 400-VCF	File Name:	828193
Nominal Diameter DN:	200 mm	Tested by:	Hochstuhl
Pressure Rating:	PN16	Weighted Mean Error (%):	0.00

Error Curve "Polynomial Correction"

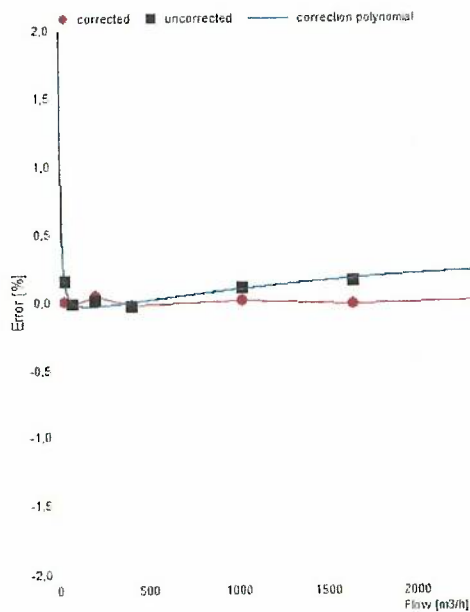

Polynomial Coefficients

am2 = -8.60967e+001
am1 = -5.17237e+000
a0 = 1.02318e-001
a1 = -2.25647e-004
a2 = 3.75911e-008

f

Qm (m³/h)	Error (%) (as found)	Error (%) (as left)
32.2	0.00	'
79.8	-0.01	'
205.4	0.04	'
410.4	-0.03	'
1028.7	0.00	'
1643.2	-0.02	'
2905	0.02	'
4151	-0.01	'

Manager of the Test Facility:

RMA Mess- und Regeltechnik GmbH & Co. KG
Forsthausstr. 3 • 77866 Rheinau
Tel. 07844 / 404-0
Steuer-Nr. 14077/22907

22.11.22 H. Hochstuhl